



Phthalate Analysis

1. Analytical Condition

YL 6500 Series

Oven : 50°C(1min)-> 30°C/min->280°C(0.1min)->15°C/min->310°C(5min)

Column : Rtx-5(30m*0.25mm*0.25um)


Carrier gas : He, 1ml/min (Split ratio 10:1)

Injector : Capillary 300°C

Detector : FID 300°C

Injection Volume : 2ul

2. Chromatogram

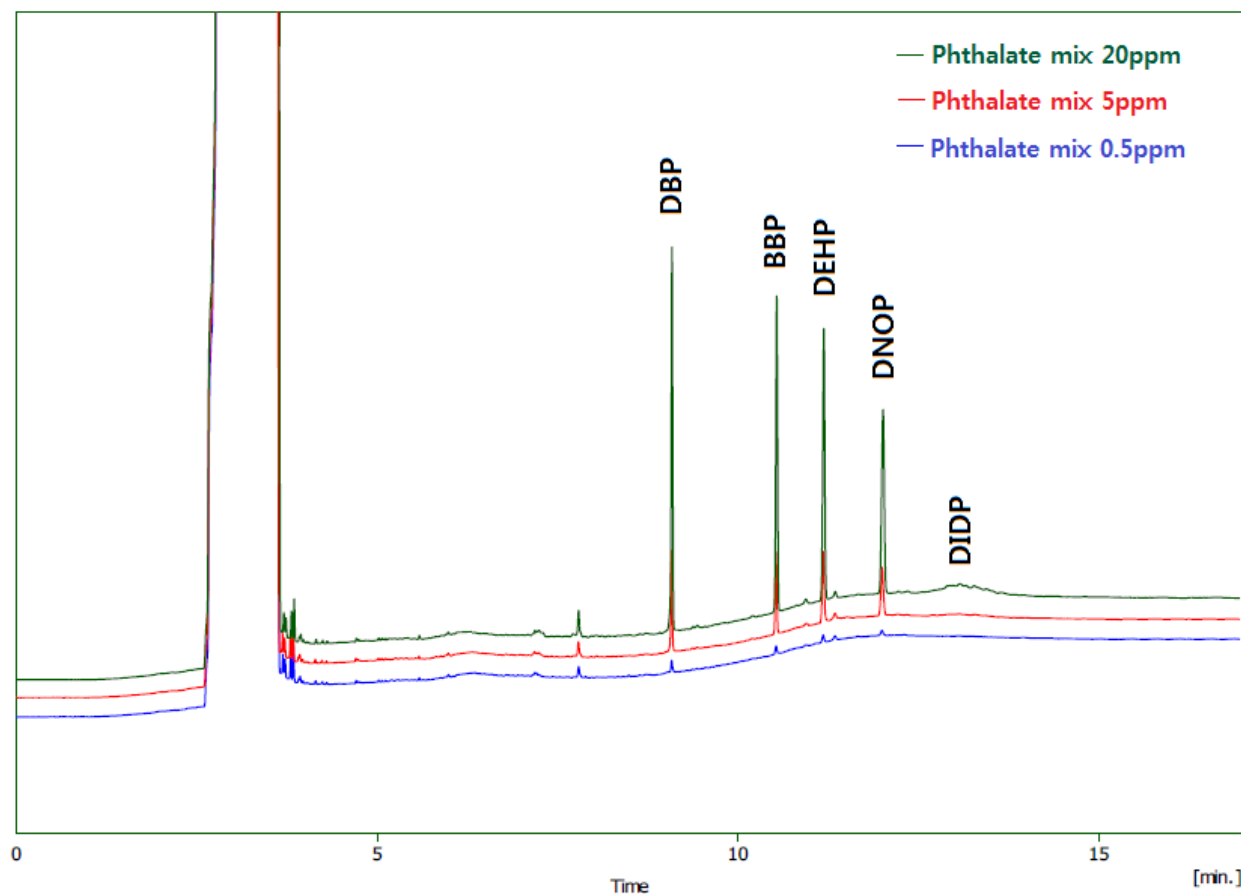



Phthalate Analysis

1. Analytical Condition

YL 6500 Series

Oven : 50°C(1min)-> 30°C/min->280°C(0.1min)->15°C/min->310°C(5min)

Column : Rtx-5(30m*0.25mm*0.25um)

Carrier gas : He, 1ml/min (Split ratio 10:1)

Injector : Capillary 300°C

Detector : FID 300°C

Injection Volume : 2ul

2. Chromatogram

